LC/MS Unknown Identifications Using MSMS Libraries
Part VI: MS Interpreter Correlation of Substructure to MSMS Ions

12/27/20

James Little
tvasailor@gmail.com
https://littlemsandsailing.com/
Kingsport, TN

- *Retired* Research Fellow, Eastman Chem. Co.*
- *42 years experience unknown identification*
- *Now Consultant, MS Interpretation Services*
- *Specialties: EI GC-MS, LC-MS/MS, Chemical Ionization, Accurate Mass, Derivatization, MS library management, SciFinder, Chemspider, Surfactant ID, NMR, GC-IR, organic synthesis, matrix ionization effects, etc.*

Eastman Chemical Company, Main Site, Kingsport, TN
50 Manufacturing Sites Worldwide, ~14,500 Employees

>50 Mass Specs Networked
Worldwide

* https://en.wikipedia.org/wiki/Eastman_Chemical_Company

Table of Contents

Topic	Slide #
Introduction of Presenter, James Little	1
Table of Contents	2
Series Topics	3
Help Files for NIST Search	4
NIST Software in General is “Windows Compliant”	5
Session Topics	6
Adding a Structure to a Spectrum	7
Sending Spectrum with Structure to MS Interpereter	9
Processing Data in MS Interpreter	10
Suggested Default Settings	11
Displaying the Propose Substructures Correlated to Ions	14
Stepping through More Than One Proposed Structure	15
Lassoing Structures Manually	16
Processing Any Entry in NIST Search with structure/spectrum	17
Direct Structure Paste in MS Interpreter	18
Processing MS/MS Spectra Containing Isotopic Clusters	19
Live YouTube Demonstration	20
References with Internet Links	21
Acknowledgements	22

LC/MS Unknown Identifications Using MSMS Libraries

Part I: Overview of Software and User Customized Configurations
Part II: NIST MSMS Search Software and Libraries
Part III: More Detailed Discussion of MSMS Hybrid Search
Part IV: Importing MSMS Spectra
Part V: NIST Structure Searches
Part VI: MS Interpreter Correlation of Substructure to MSMS Ions
Part VII: Using and Creating Other MSMS Libraries
Part VIII: Identification of Unknowns with "Spectraless" Libraries
Part IX: Using Agilent MassHunter with NIST MSMS Search

Help Files for NIST Search

-"Hover" over Program Icon with mouse and function description displayed

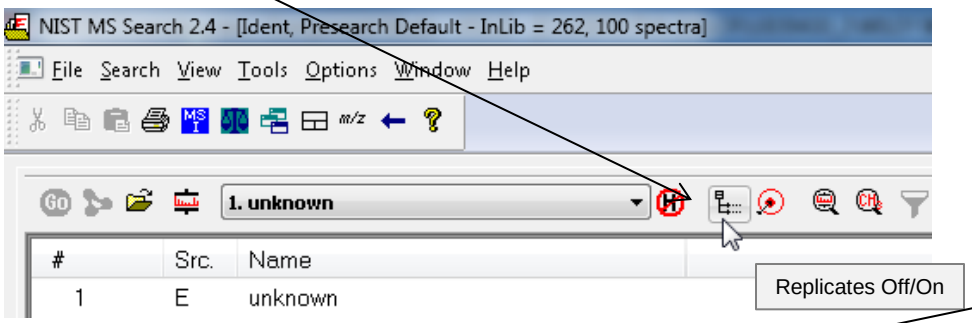

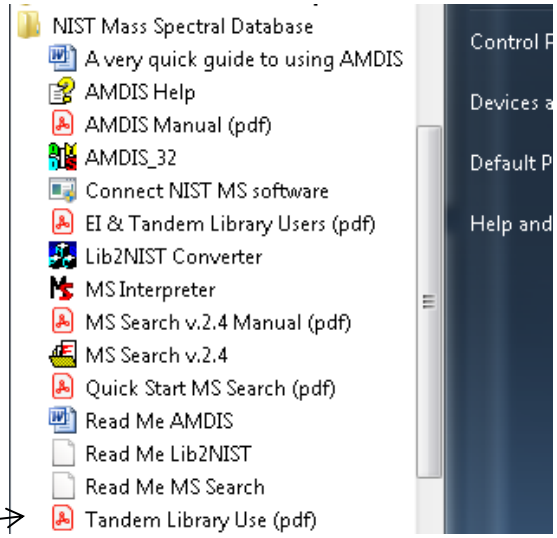

-***Detailed*** documentation for NIST Search[8]
-MS Interpreter included in NIST manual[8]
-Windows Program Group
-NIST Tandem Search ***Quick Start Guide***[9]
-"In program" assistance for both programs
-***Help button*** at corner of all windows

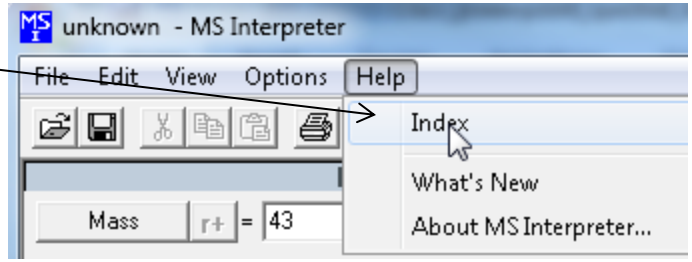

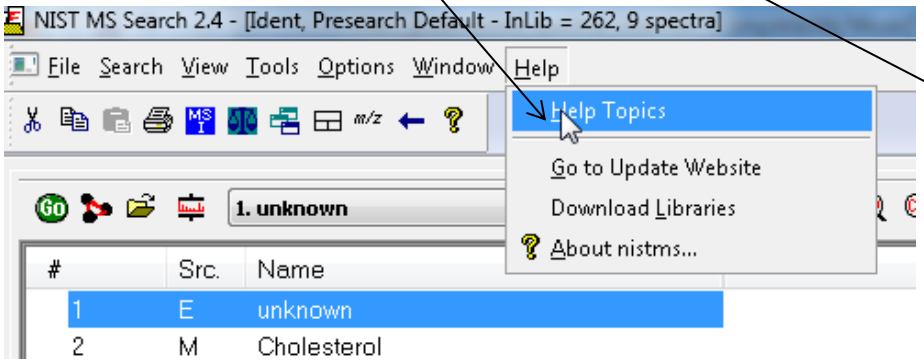

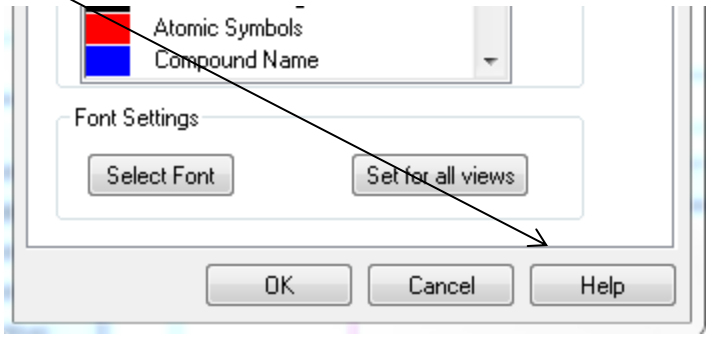

NIST Software in General is "Windows Compliant"

-***left click (LMB)*** to select an item, ***double LMB*** on that item to perform operation
-***right click (RMB)*** in area or item to see operations that can be performed or to change properties of window
-***LMB*** on first item and last item to select group ***while*** holding ***shift key***
-***LMB*** to select/deselect individual items ***while*** holding ***Ctrl button***
-use up and down arrows ***on keyboard*** to step between entries
-some NIST windows such as librarian have no delete button to delete ions, ***must*** use delete key on keyboard!
-***control a*** (select all), ***control x*** (delete selected), ***control c*** (copy); ***control v*** (paste)
-***control k*** copies entries into windows in tab-separated text format, e.g., ***paste*** into Excel
-F1 MS Search help
-F9 send spectrum to MS Interpreter

Tip 3: ***LMB*** and **drag** to rearrange order of column headers

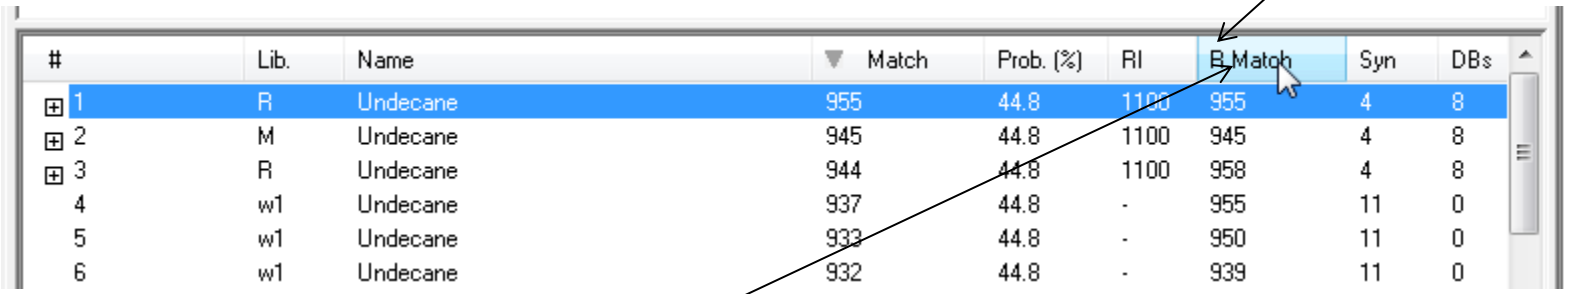

#	Lib.	Name	Match	Prob. (%)	RI	R.Match	Syn	DBs
1	R	Undecane	955	44.8	1100	955	4	8
2	M	Undecane	945	44.8	1100	945	4	8
3	R	Undecane	944	44.8	1100	958	4	8
4	w1	Undecane	937	44.8	-	955	11	0
5	w1	Undecane	933	44.8	-	950	11	0
6	w1	Undecane	932	44.8	-	939	11	0

-***LMB*** on column of interest
-Can sort in lower value first or higher

Tip 1: When reviewing search results, use up and down arrows on keyboard to quickly step through results!

Tip 2: When viewing structures in MS Interpreter, use left and right arrows on keyboard to quickly review results!

Part VI: MS Interpreter[9-12] Correlation of Substructure to MSMS Ions

Session Topics:

-Setting up ***Library Search Options*** MS Interpreter
-Associating structure with spectrum
-Processing data

MS Interpreter for Correlating Structure to Spectrum:

Adding a Structure to a Spectrum

1) ***Import*** the mass spectrum from instrument data system
2) ***Open Librarian tab*** at bottom of MS Search Window
3) ***View*** in ***Librarian*** tab

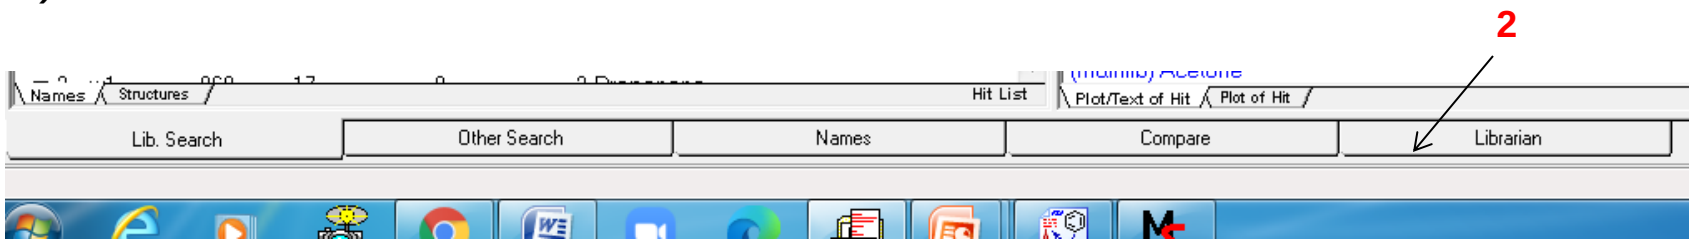

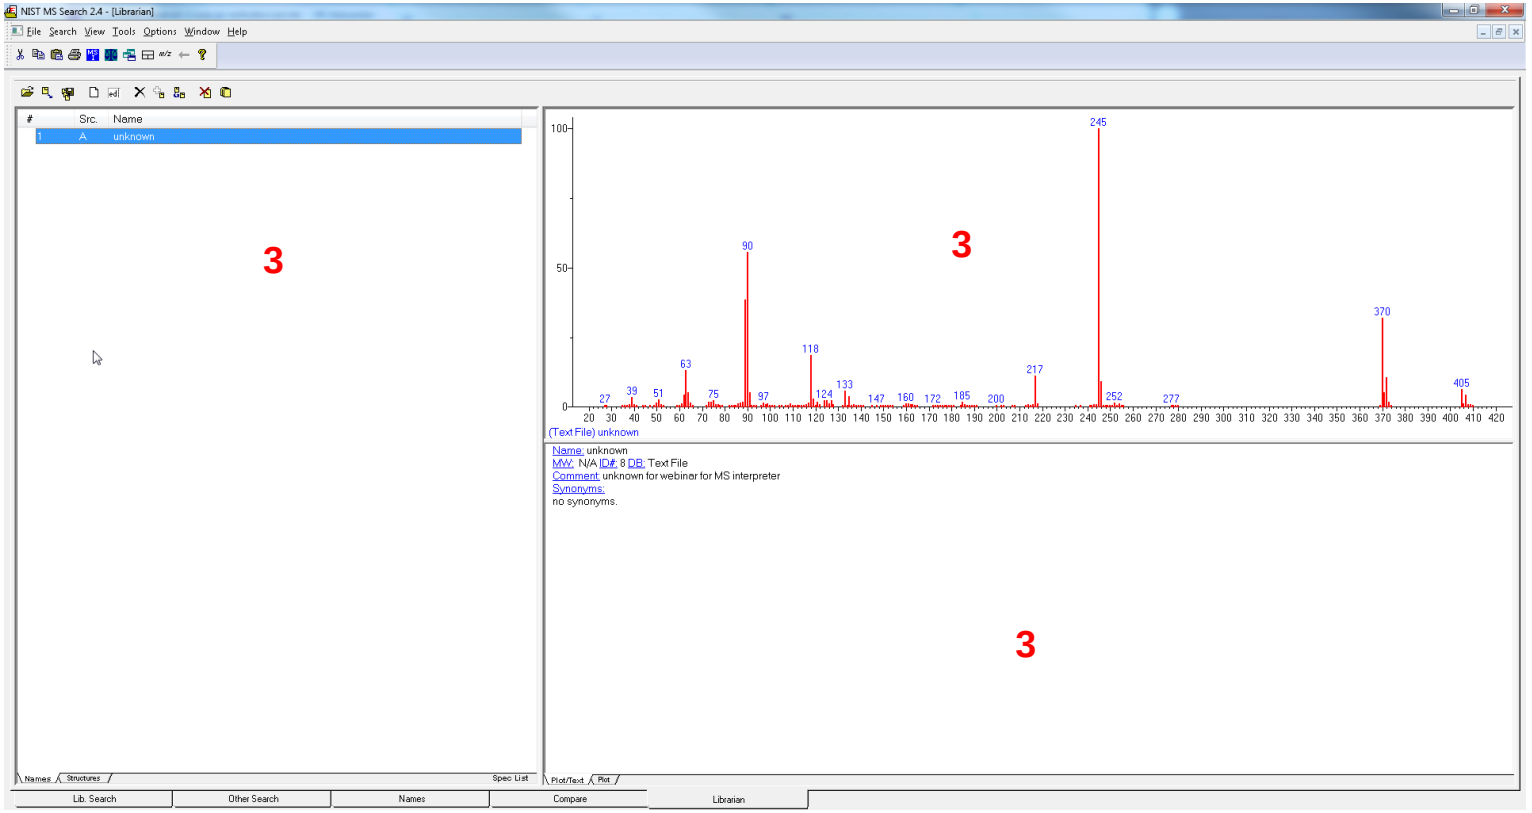

MS Interpreter for Correlating Structure to Spectrum:

Adding a Structure to a Spectrum

1) ***Draw*** the proposed structure with drawing program and ***copy*** into clipboard
2) ***Open Librarian tab*** and select ***"ed "*** icon with **left mouse click**
3) ***LMB*** on **From Clipboard** to associate structure with spectrum
4) ***Modify*** name fields, synonyms, comments fields, or even ***edit*** spectrum
5) ***Add to List***

Tip: This is basically the approach used to ***create a user library*** and/or user library ***entry***. This will be discussed in detail in Presentation VII in this series. ***Instead*** of "Add to List", the "Add to library" button will be selected. Also, one can "Replace" a current spectrum in user library after correcting it.

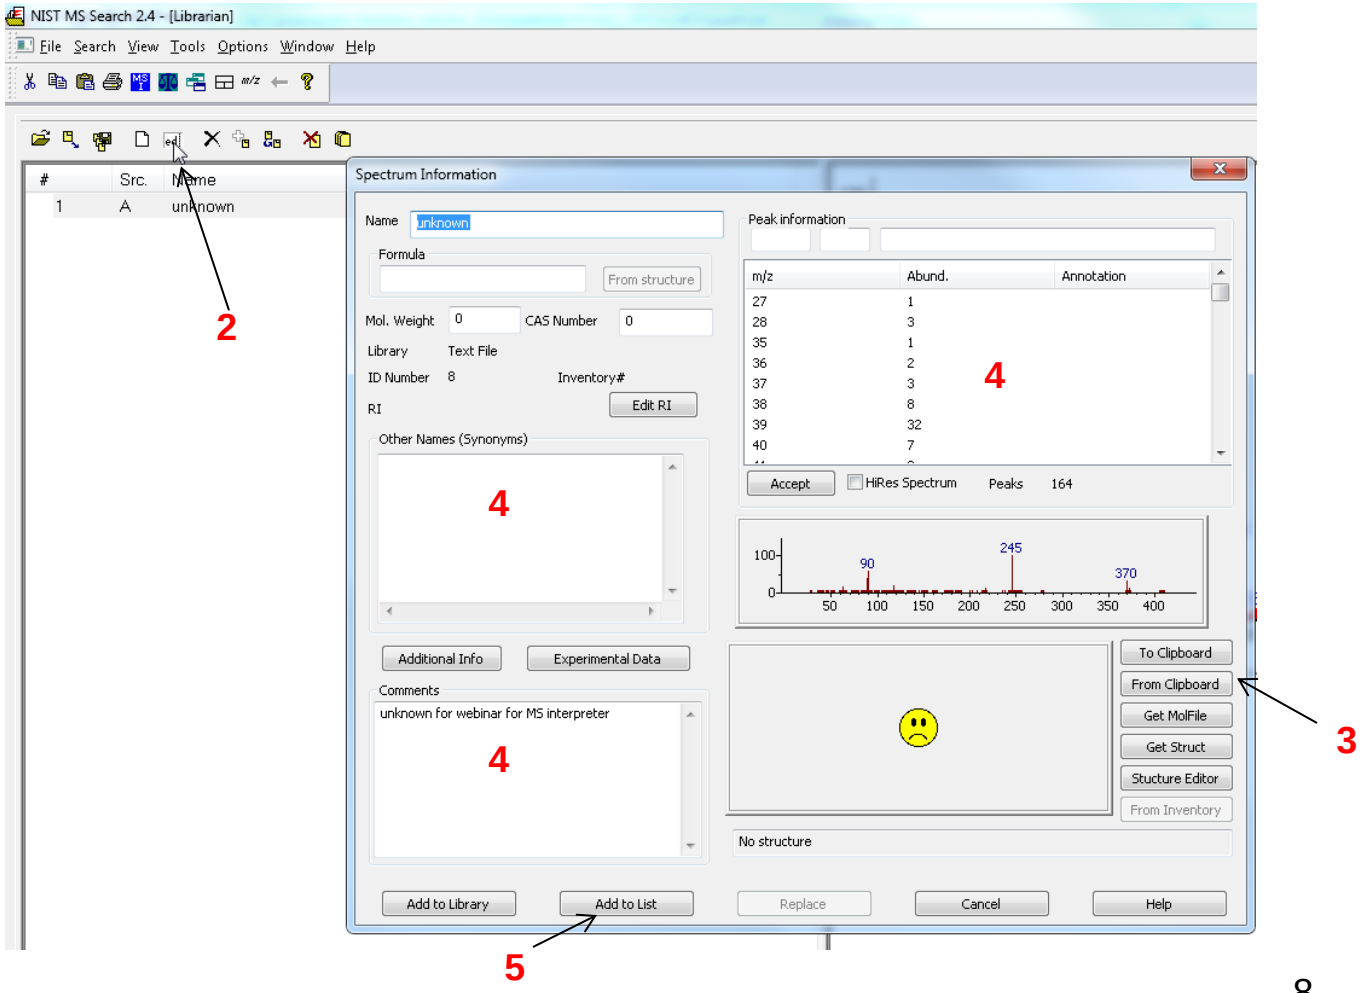

MS Interpreter for Correlating Structure to Spectrum:
Sending to MS Interpreter

1) Entry is now ready to send to MS interpreter
2) Program has automatically calculated nominal molecular weight, exact mass, molecular formula, and InChIKey
3) ***Right mouse*** click on selected entry, then LMB on Send to/MS Interpreter
4) An ***alternative*** to step 3, is to ***send*** the entry to MS interpreter ***using F9*** key

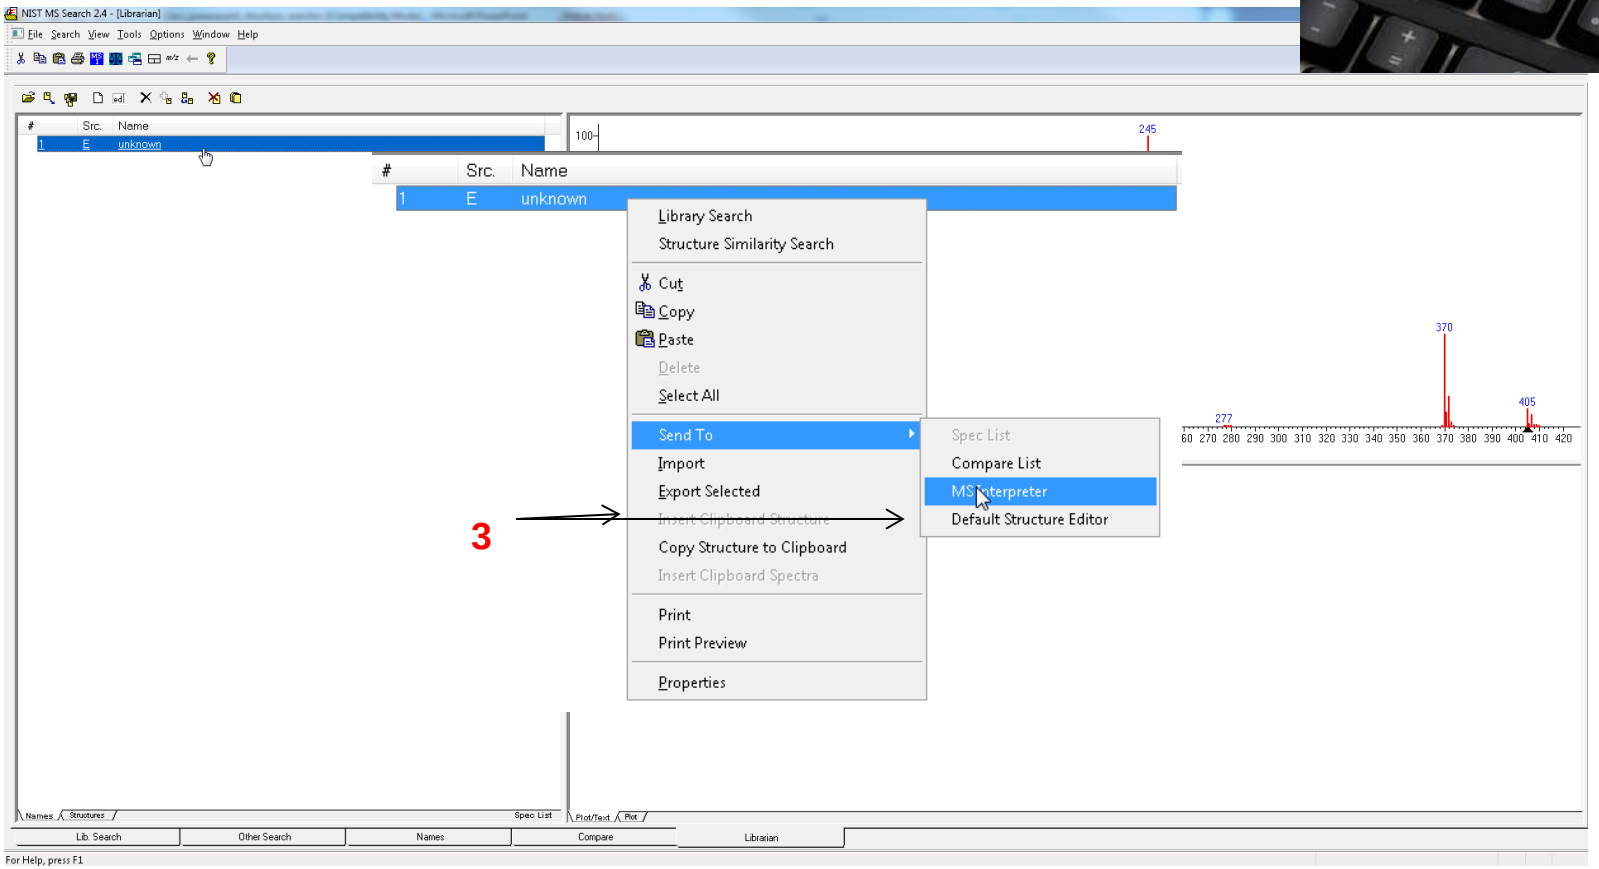

MS Interpreter for Correlating Structure to Spectrum:

Processing Data in MS Interpreter

-All ions in black, yellow, and red correlated to structure automatically
-Ions in white are not assigned
-Spectrum can be expanded like any spectrum in NIST programs by ***LMB*** and ***dragging*** to form box
-***RMB*** and then ***LMB Unzoom*** to return to original size

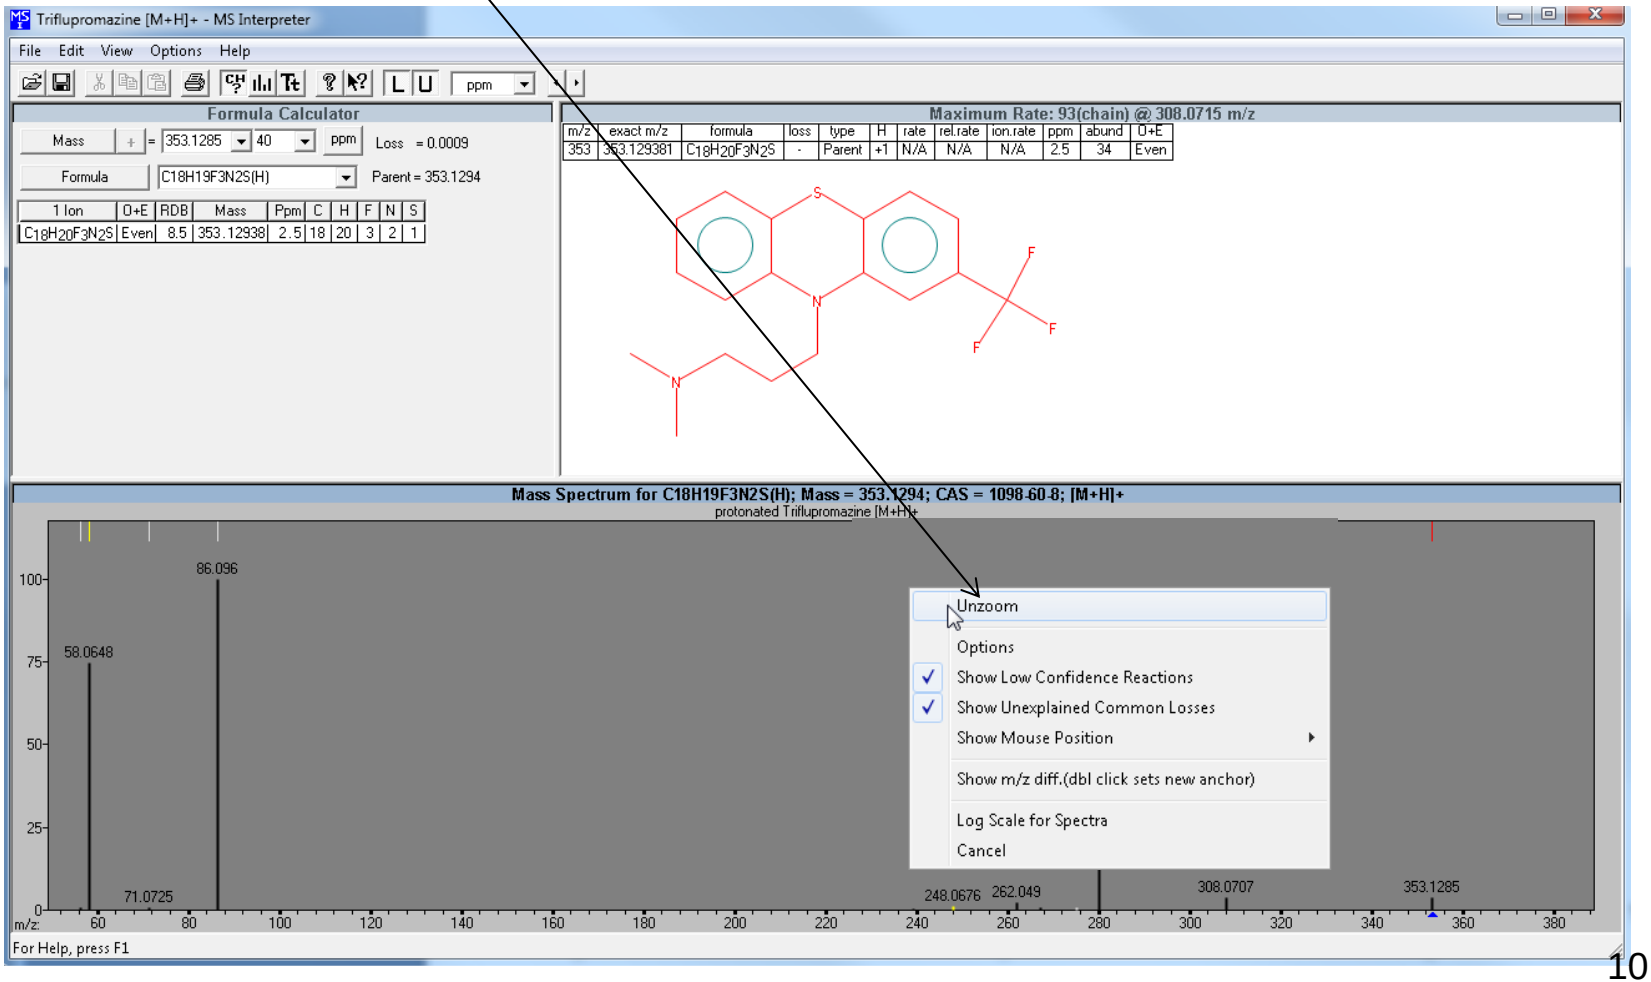

MS Interpreter for Correlating Structure to Spectrum:

Suggested Default Settings for MS/MS (Tandem)

1) Select **Options** with **LMB** click then **Fragmentation options**
2) Setup options as noted in window
3) ***In this case***, “Protonated”, if M-H, select “Deprotonated”

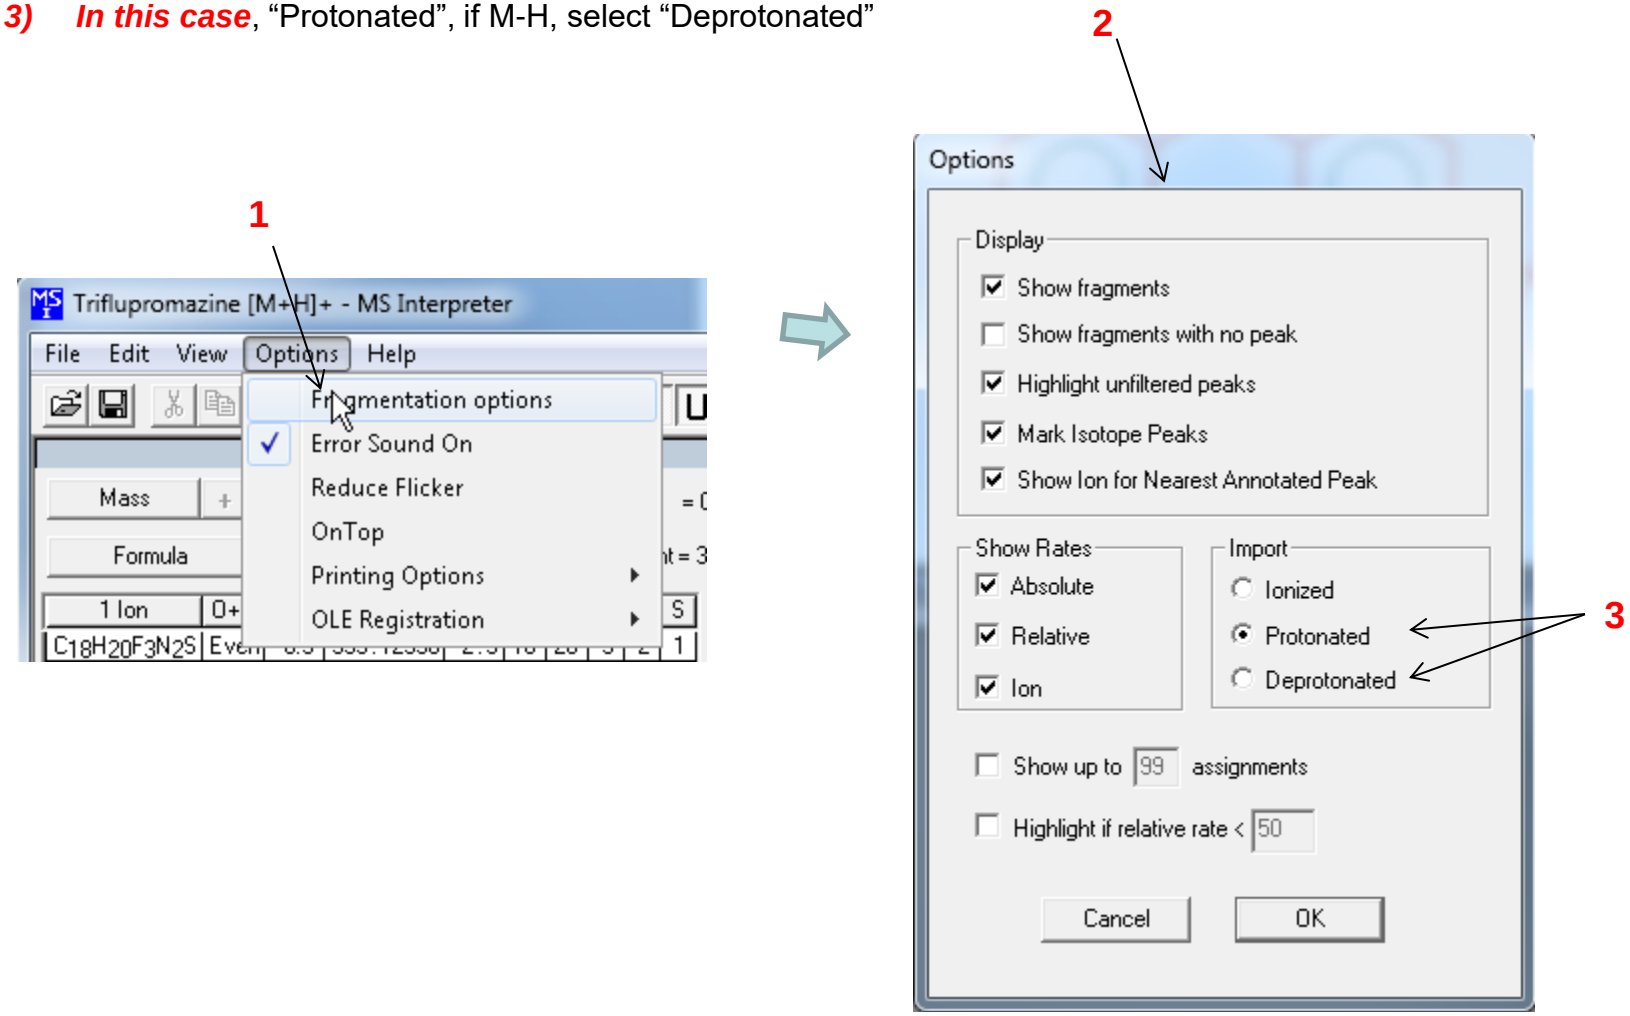

MS Interpreter for Correlating Structure to Spectrum:

Suggested Default Settings for MS/MS (Tandem)

1) Select ***Isotopes Calc*** icon ***if your*** spectrum has isotopes
2) Select the Defaults as appropriate
3) This spectrum has ***no*** isotopes, just precursor

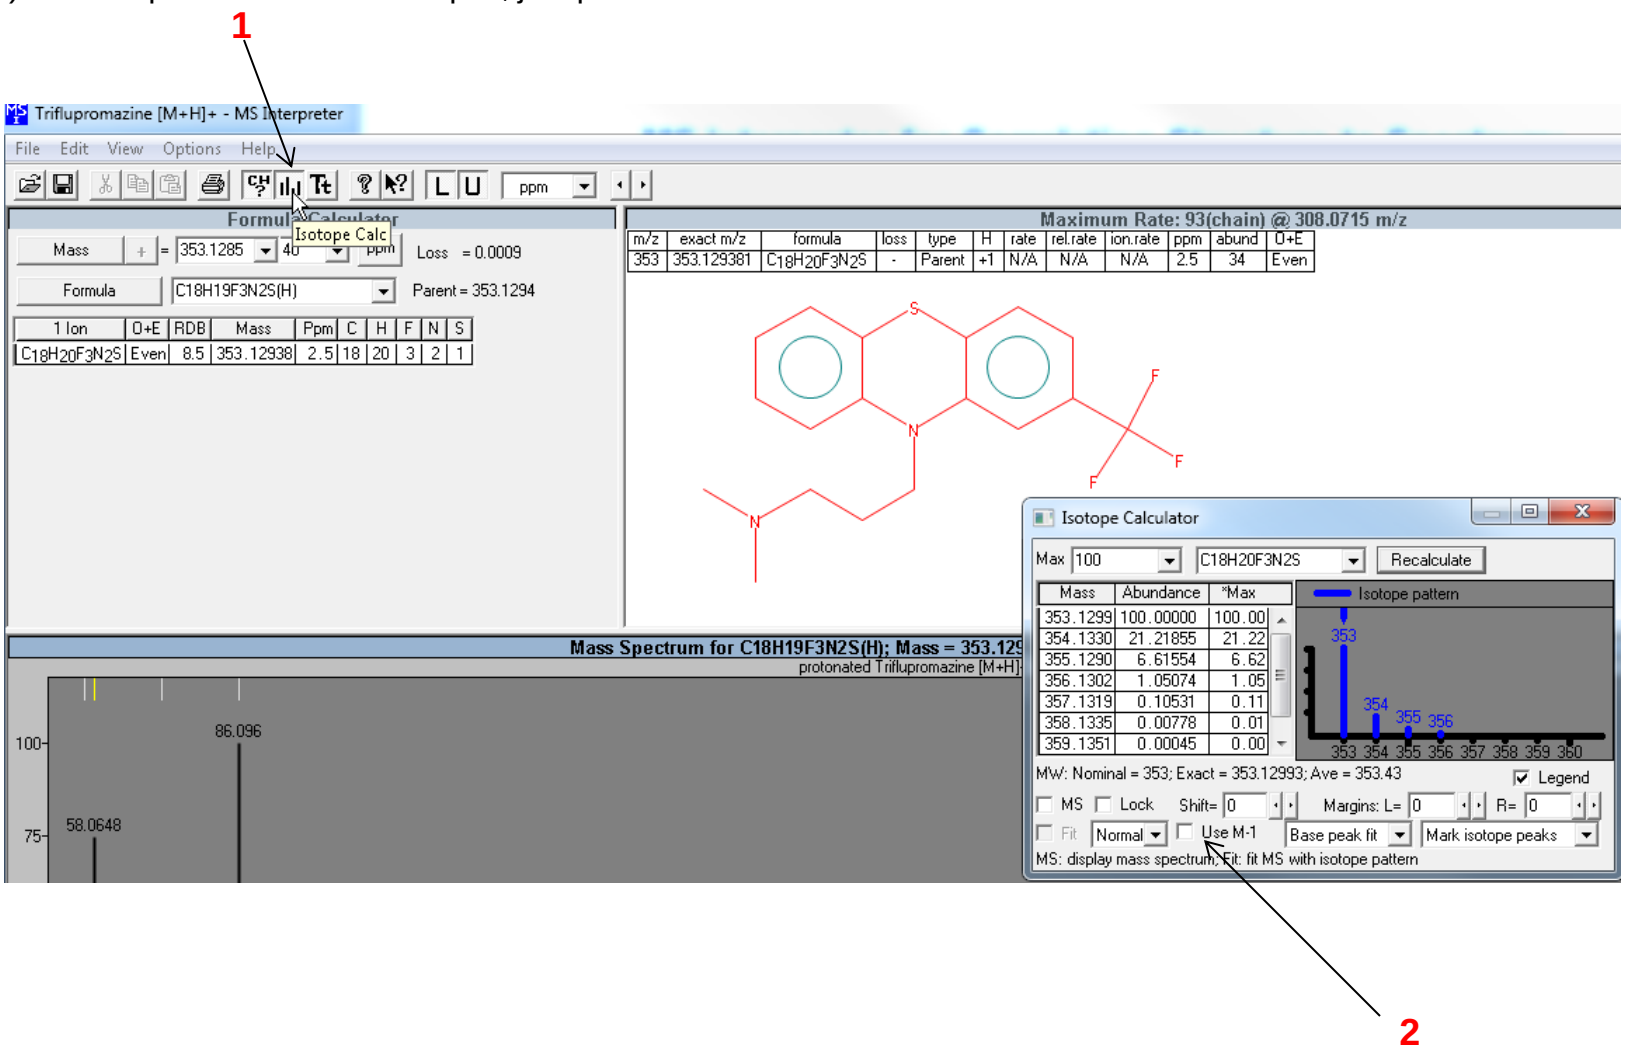

MS Interpreter for Correlating Structure to Spectrum:

Suggested Default Settings for MS/MS (Tandem)

1) ***RMB*** in spectrum window, then ***LMB*** to select ***Show Mouse Position/On Cursor***
2) ***Formula Isotope button depressed*** to display window, also Formaula Isotope Calc if appropriate
3) ***Low confidence mechanism*** and ***unknown mechanism*** buttons ***depressed*** to show additional fragmentation

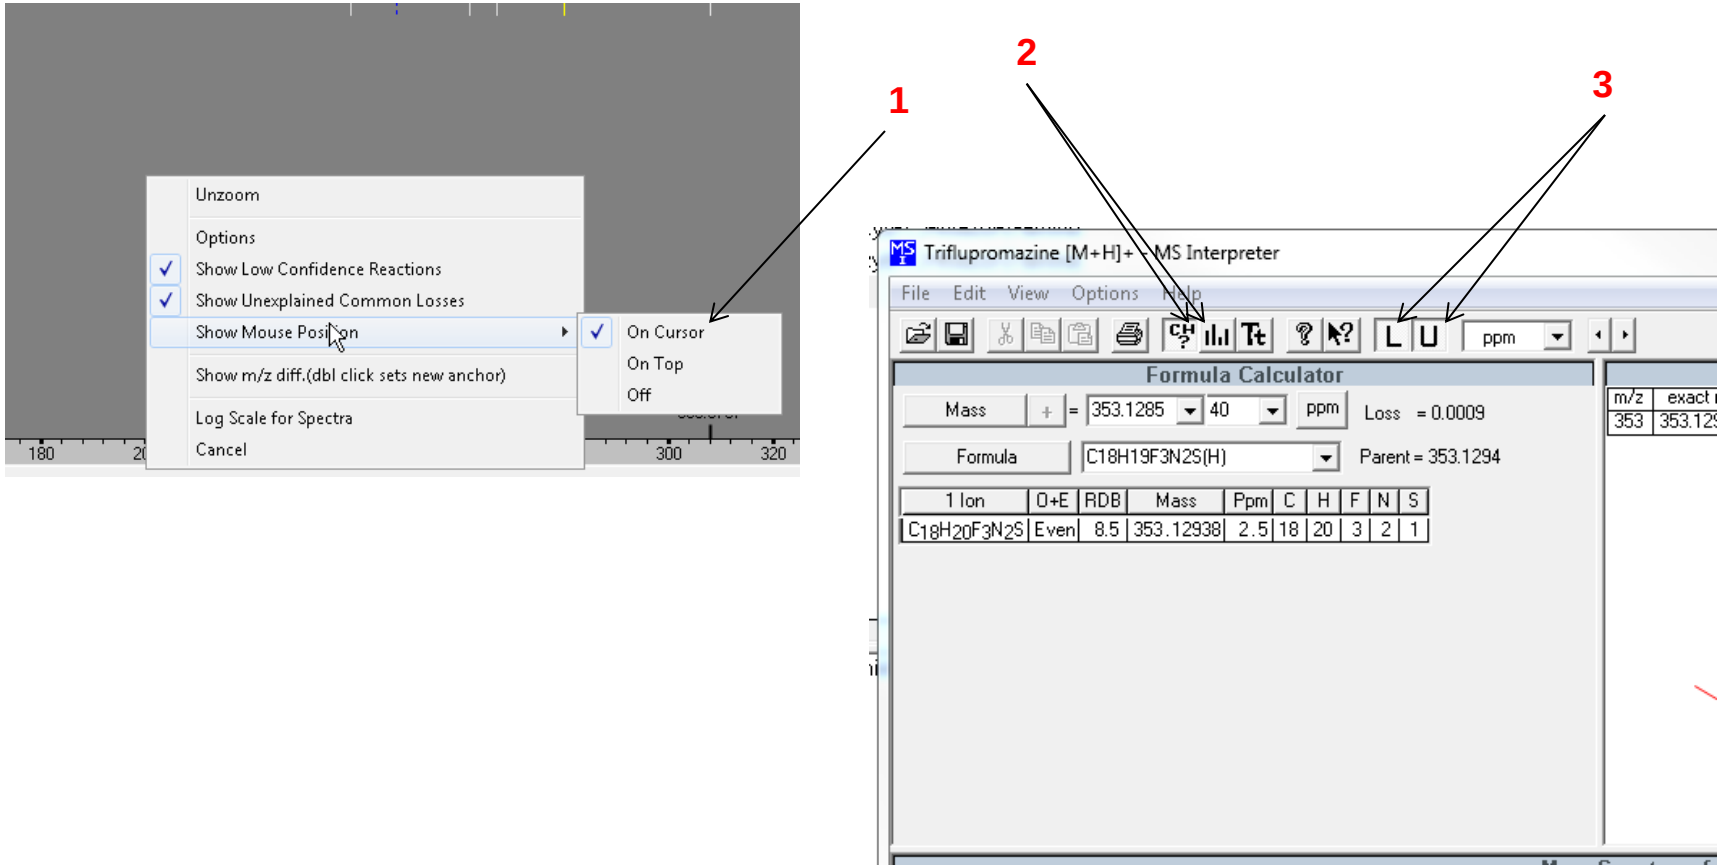

MS Interpreter for Correlating Structure to Spectrum:

Displaying the Proposed Structures

1) ***LMB*** on the ion of interest and the
2) Structure in ***highlighted in red*** in top window

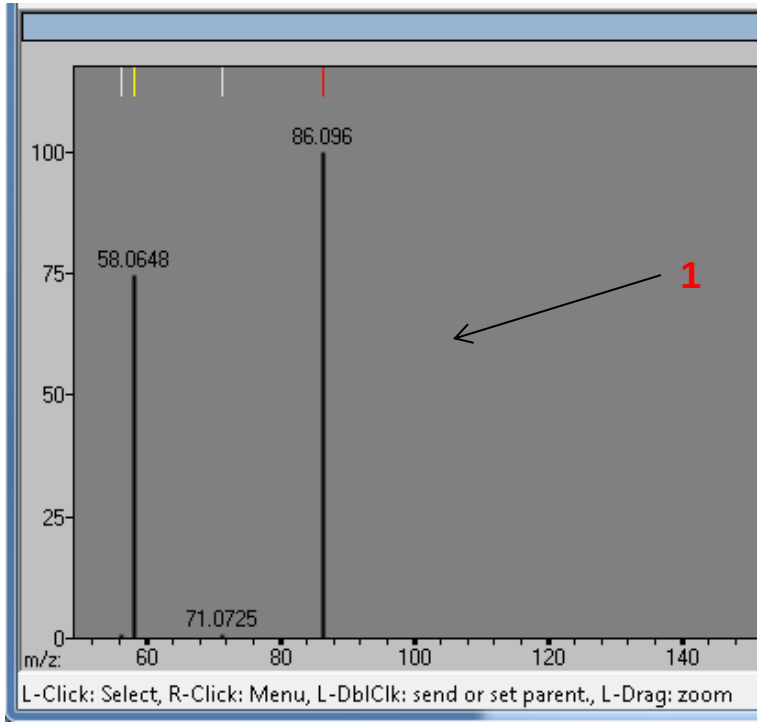

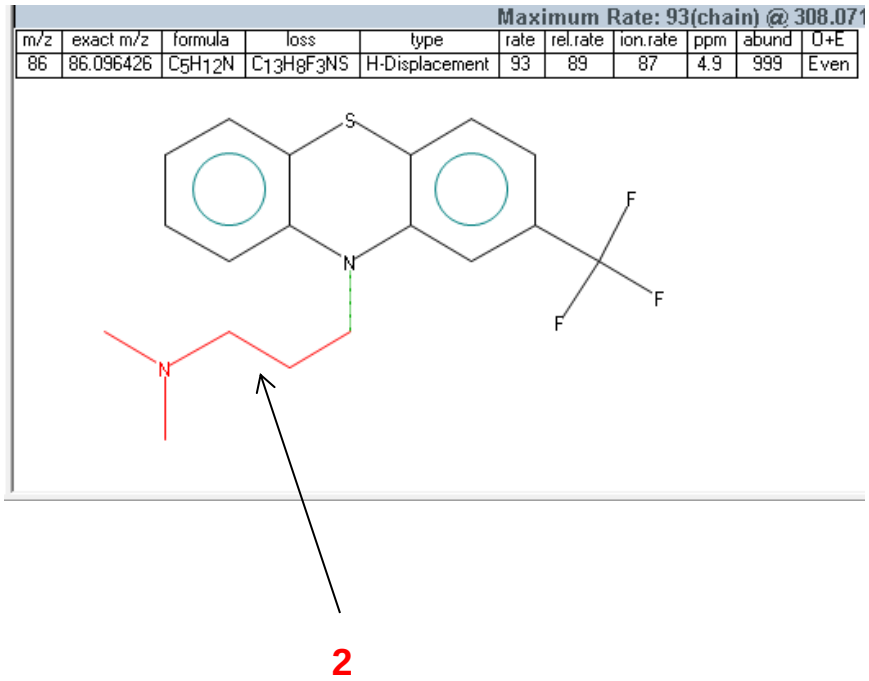

MS Interpreter for Correlating Structure to Spectrum:

*Stepping Through **More** Than One Proposed Structure*

1) ***LMB*** on the ***tick mark*** for ion of interest , the display will toggle through ***all 4*** in this example

2) If ***more than one*** is present, the box will indicate the number, in this case ***¼***

3) Also, you can select one of the tick marks with LMB then use your ***left*** and ***right*** arrows ***on keyboard*** to step through the assigned ions in the mass spectrum

1

click on tick marks

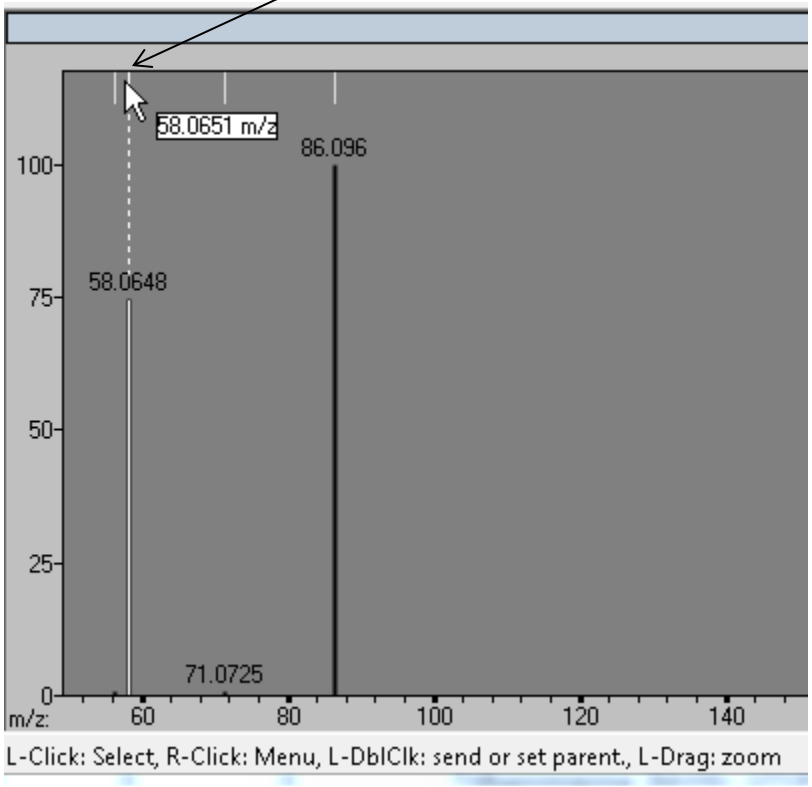

2

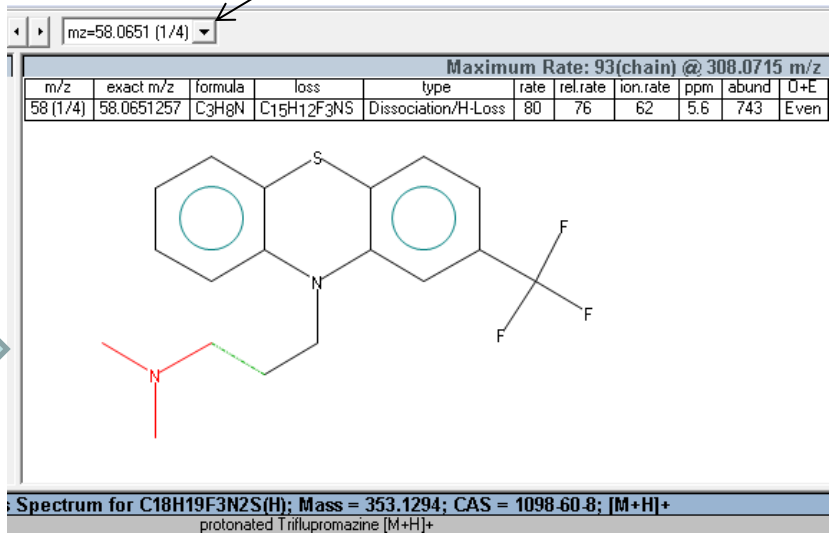

3

MS Interpreter for Correlating Structure to Spectrum:

Other Miscellaneous Tips: Lassoing Ions Manually

1) ***Lasso*** your own substructure by ***LMB*** and ***circling,*** shows type as ***highlighted***

2) The formula , exact mass, and loss will be shown in the “Formula Calculator” window

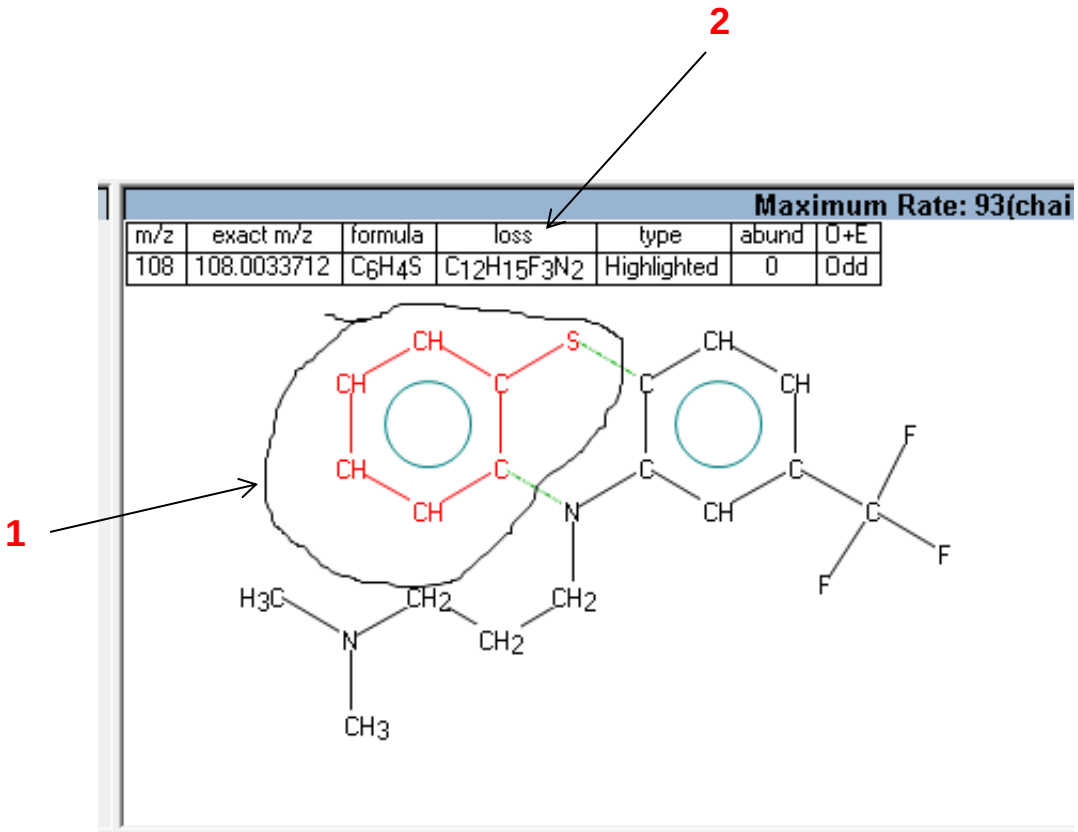

Any Structure and *Associated Spectrum* in NIST Program Can be *Sent* to *MS Interpreter*

1

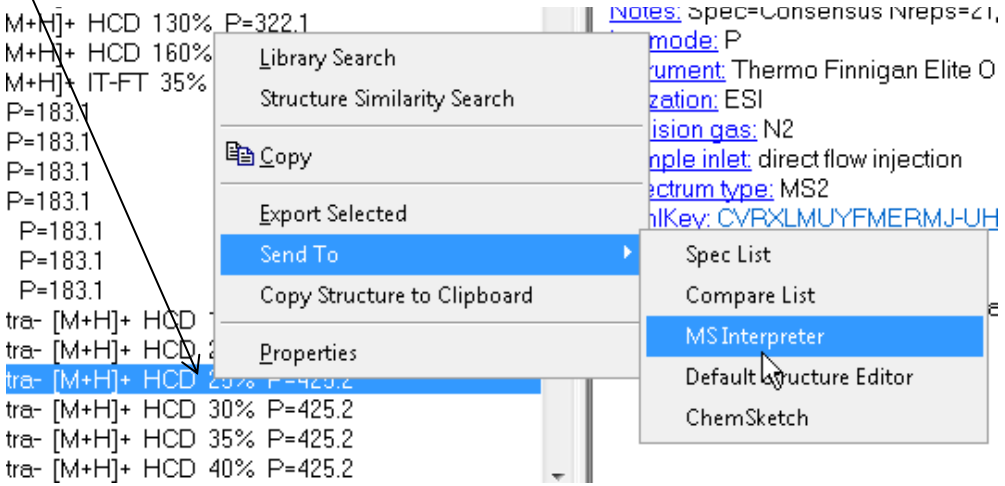

1. ***Either*** ***LMB*** select then ***RMB*** **Send To/MS Interpreter**
2. ***Or*** select ***F9*** on keyboard

2

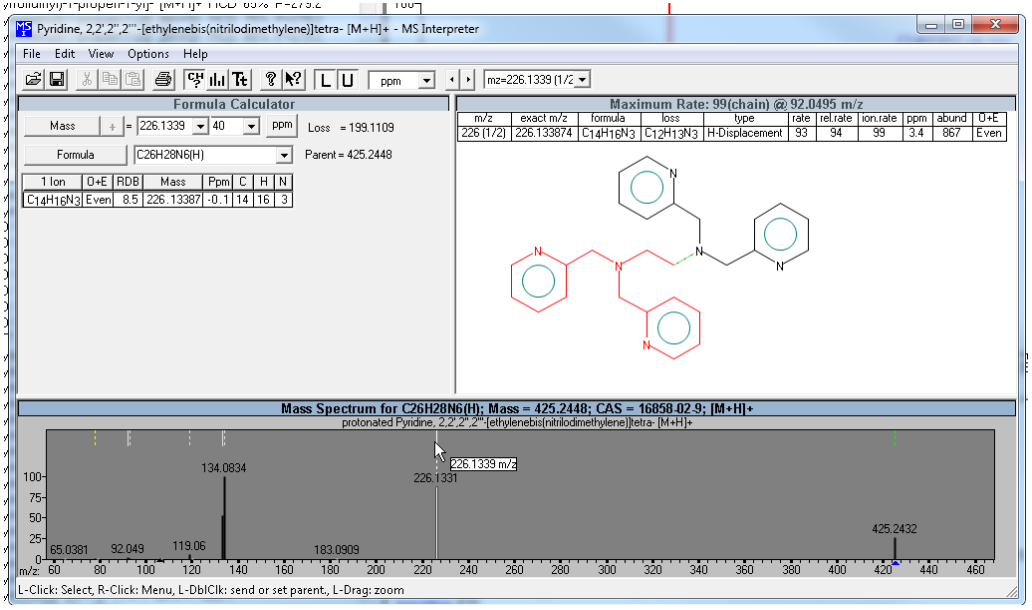

MS Interpreter for Correlating Structure to Spectrum:

Other Miscellaneous Tips: Direct Structure Paste

1) ***Copy structure*** into clipboard ***from drawing program***, then ***directly paste*** into MS interpreter with control V on keyboard or ***pull-down menu/paste***

2) The structure ***cannot be saved*** with spectrum upon exiting MS Interpreter

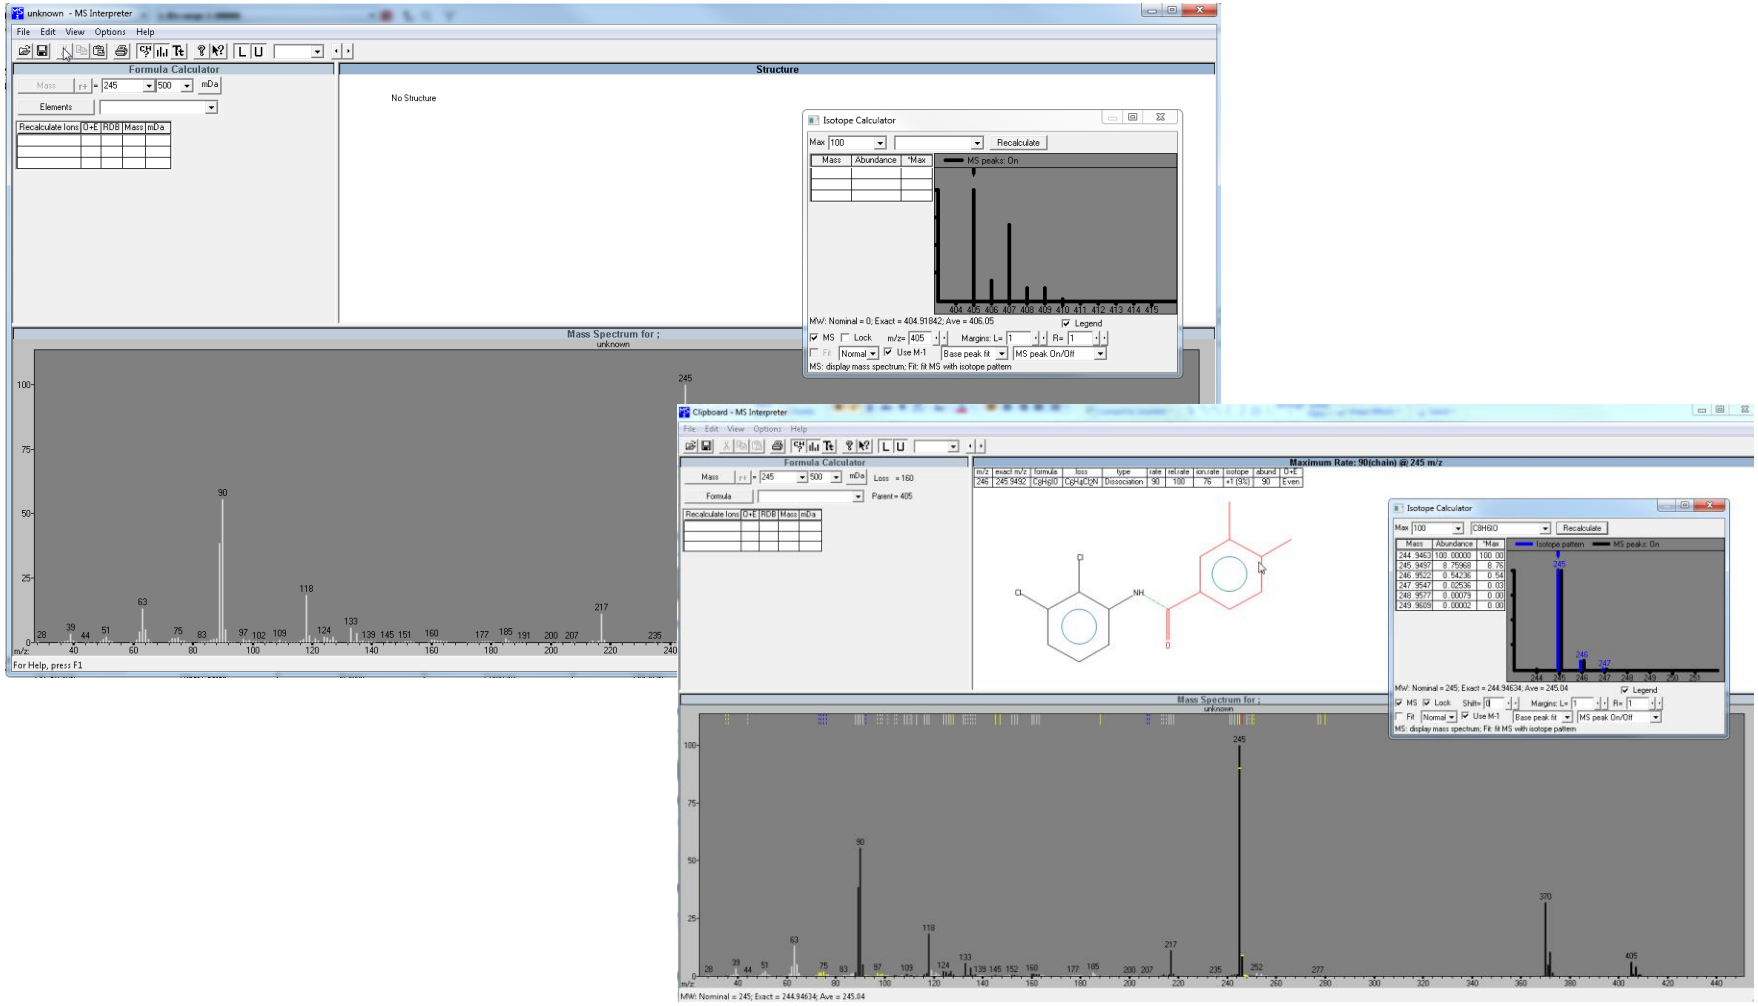

MS Interpreter for Correlating Structure to Spectrum:

If your MS/MS (Tandem) Spectrum is acquired with isotopes

1) ***RMB*** on the formula for the ion, then ***LMB*** on ***Send "x" to Isotope Calc***

2) Theoretical isotope ratio ***compared*** to observed

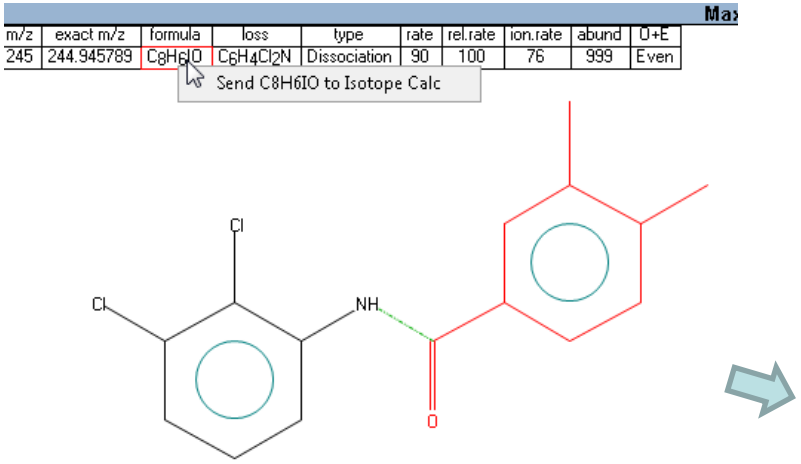

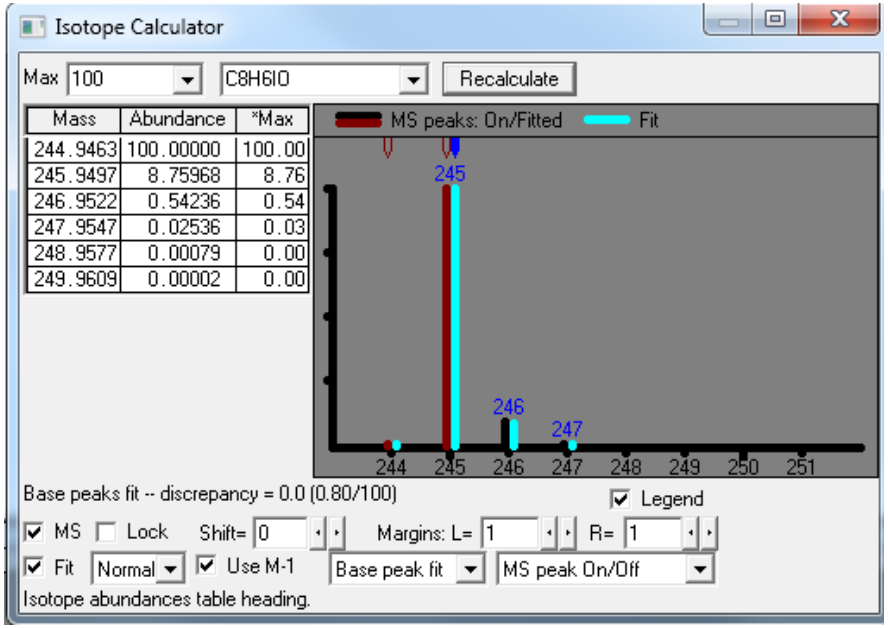

Live Demo on YouTube
LC/MS Unknown Identifications Using MSMS Libraries
NIST Structure Searches

Acknowledgements

- Stephen Stein (NIST)
- Alexey Mayorov (NIST)
- Yuri Mirokhin (NIST)
- Dmitrii Tchekhovskoi (NIST)
- David Sparkman (NIST consultant)